



Positive Control –


eae

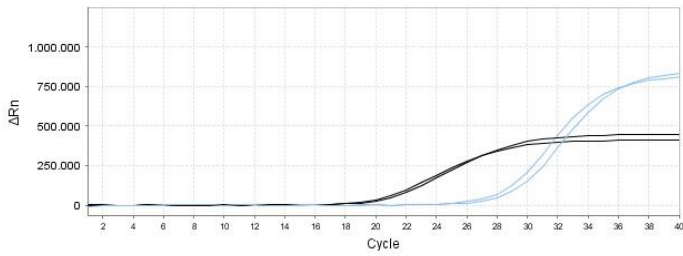

vtx1

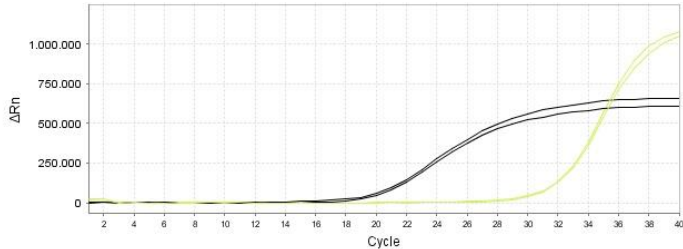


vtx2

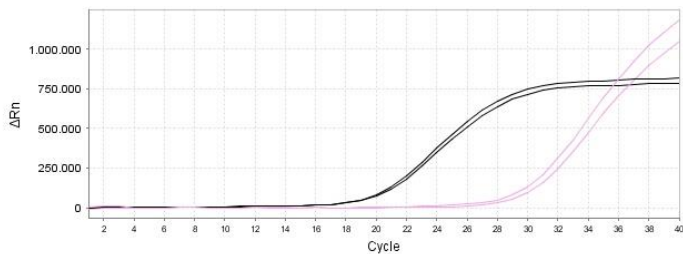

Negative Control –

Amplification Plot

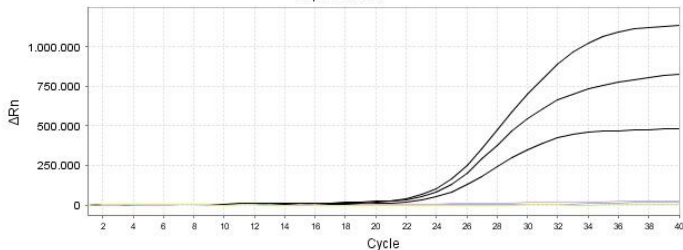

12. SPECIFICITY/INCLUSIVITY

- 100 % Exclusivity, determined using 30 strains of closely related organisms or occurring in the same habitat.
- 100 % Inclusivity, determined in 18 positive samples for *eae*, *vtx1* and/or *vtx2* genes of *Escherichia coli*.

13. SENSITIVITY

A detection Limit of 1 to 10 cells per 25g of food sample can be achieved after enrichment. The REAL TIME DETECTION KIT *E. coli* EPEC, VTEC and EHEC detects down to 10^3 - 10^4 cfu/mL in enrichment cultures. This kit has a reaction sensitivity of 25 pg of target DNA.

REAL TIME DETECTION KIT

E. coli - EPEC, VTEC and EHEC

Ref: BIOPFS-0002

1. PRODUCT DESCRIPTION

Pathogen detection kits provide a simple, reliable, and rapid procedure for detecting the presence of a specific pathogen. The assay is based on 5' nuclease real time PCR reactions to amplify a unique genomic sequence in the target microorganism.

2. TECHNOLOGY DESCRIPTION

PCR is a method used to amplify a specific DNA sequence in a reaction containing among other components, a thermostable DNA polymerase, nucleotides, and primers complementary to the target sequence. The DNA molecule denatures when this solution is heated, separating into two strands. As the solution cools, the primers anneal to the target sequences in the separated DNA strands and the DNA polymerase synthesizes a new strand by extending the primers with nucleotides, creating a copy of the DNA sequence (amplicons). When repeated, this cycle of denaturing, annealing, and extending exponentially increases the number of target amplicons. In Real Time PCR, the signal is measured in each cycle, using in most cases specific fluorescent probes. Fluorescence is measured by a detector and the associated software plots the fluorescence intensity versus the number of cycles, allowing the determination of the presence or absence of the target organism.

3. PATHOGEN DESCRIPTION

Escherichia coli, which is part of the microbiota of the intestine, can cause enteric/diarrhoeogenic or extra-intestinal infections in humans. Enteric *E. coli* that cause disease can present different virulence determinants, corresponding to different pathotypes. These include the verocytotoxigenic *E. coli* (VTEC), comprising the enterohaemorrhagic *E. coli* (EHEC), and the enteropathogenic *E. coli* (EPEC). VTEC are characterized by the production of verocytotoxins (Vtx), encoded by *vtx1* or *vtx2* genes, (also known as Shiga-like toxins - Stx - corresponding to *stx1* and *stx2* genes). EHEC are a subset of VTEC, that in addition to the Vtx-encoding genes carry the attaching and effacing gene *eae* (intimin-coding) and have the ability to cause attaching and effacing lesions in hosts. EPEC carries the *eae* gene but does not produce Vtx. EHEC strains are typically isolated from cases of severe disease like diarrhea, hemorrhagic colitis (HC) and the potentially fatal hemolytic uremic syndrome (HUS). These *E. coli* strains, especially EHEC (including the O157:H7 and O157:H-serotypes), are recognized as major pathogens of foodborne disease in humans. They are mostly transmitted through undercooked minced beef, inadequately pasteurized milk, cold sandwiches, sprouts, and vegetables. The need for rapid, accurate, and sensitive methods for the detection of these *E. coli* strains is a major food safety issue. Since conventional microbiological methods for their detection and identification are time-consuming, PCR has been introduced to the food industry as a highly sensitive and specific detection method.


4. INTERNAL CONTROL (IC)

Pathogen detection kits include an Internal Control (IC) in the master mix. This control is amplified at the same time as the target DNA sequence, but using a different set of primers and a probe labeled with a different fluorophore. The inclusion of the IC in each reaction allows the evaluation of PCR inhibitors in negative results.

5. APPLICATION

REAL TIME DETECTION KIT *E. coli* EPEC, VTEC and EHEC is intended to rapidly detect *E. coli* EPEC, VTEC and EHEC in food samples, after enrichment in buffered peptone water and DNA extraction. It can also be used with animal feedstuff and environmental samples. The kit was validated in the instruments ABI PRISM® 7500 Fast and ThermoScientific® PikoReal. The kit is compatible with all thermocyclers working in **FAM** and **ROX** channels. The detection kit must not be used for diagnostic procedures. For Food use only.

The procedure includes the following main steps:



Sample
Enrichment

DNA
extraction

PCR
set-up and run

Results and
Interpretation



BPMPR – Production and Development, Lda. Amadora INOVA
Rua Henrique de Paiva Couceiro, 10
2700 – 453 Falagueira – Venda Nova Amadora, PORTUGAL
Tel: +351 211 451 410
E-mail: sales.support@biopremier.com
Website: <http://www.biopremier.com>

BPMPR is certified ISO 9001:2015

6. CONTENTS AND STORAGE

The kit contains reagents for 50 assays for each target

CONTENTS	UNITS	COMPOSITION
Master Mix (blue cap)	3 tubes (3 x 840 µl)	Buffer, dNTPs, DNA polymerase
Assay Mix – <i>eae</i> (brown cap)	1 tube (1 x 105 µl)	Primers and Probes
Assay Mix – <i>vtx1</i> (brown cap)	1 tube (1 x 105 µl)	Primers and Probes
Assay Mix – <i>vtx2</i> (brown cap)	1 tube (1 x 105 µl)	Primers and Probes
Negative Control (clear cap)	1 tube (1 x 105 µl)	Nuclease-free water
Positive Control (red cap)	1 tube (1 x 105 µl)	Target DNA

Store all contents at -20°C and protect them from light as excessive exposure to light may affect the fluorescent probes. Minimize freeze-thaw cycles. Reagents stored as recommended may be used until the expiration date indicated in the tube.

7. MATERIAL REQUIRED AND NOT SUPPLIED

- Microcentrifuge
- Laminar Air Flow Cabinets/PCR Cabinets
- Disposable powder-free gloves
- Micropipettes and nuclease-free filter tips
- Real-time PCR instrument
- Tubes/Strips/Multiwell plates and accessories specific for each Instrument
- Lysis buffer / DNA extraction kit (example: BIOPEXT-0400/ BIOPEXT-0609).

8. PRECAUTIONS AND RECOMMENDATIONS

Molecular Biology procedures, such as DNA extractions and PCR amplification, require qualified staff to prevent the risk of erroneous results, especially due to sample contamination or degradation of the nucleic acids contained in the samples. It is strongly recommended to have dedicated areas, materials, and equipments for the DNA extraction, preparation of the PCR and post-PCR procedures. Workflow in the laboratory must proceed in a unidirectional manner, beginning in the Extraction Area and moving to the Amplification and Detection Area.

The user should always pay attention to the following:

- Read all the instructions provided before running the assay.
- Do not mix reagents from different batches.
- Wear proper PPE, including disposable gloves and laboratory coats.
- Store and extract positive material separately from all other reagents.

9. QUALITY CONTROL

In accordance with BPMR's ISO 9001, each lot of the kit is tested against predetermined specifications to ensure consistent product quality.

10. PROCEDURE

10.1 Enrichment

Recommended a pre-enrichment according to ISO 16654:2001, BAM (Chapter 4a) or USDA for 18 - 24 h. Other suitable, validated enrichment procedures can also be used.

10.2 DNA extraction

1. Collect 1 mL of enriched sample and centrifuge at 10,000 - 12,000 g for 5 min.
2. Discard all the supernatant.
3. Wash the pellet: add 1 mL of 0.9% NaCl solution or PBS.
4. Centrifuge at 10,000-12,000 g for 5 min and discard all the supernatant.
5. Use a kit or suitable protocol for DNA extraction. Such as BIOPREMIER DNA Rapid Extraction Buffer (ref: BIOPEXT-0400) or BIOPREMIER DNA Extraction Kit from Food (ref: BIOPEXT-0609) (not included).

10.3 PCR preparation

A – PCR mix

Always wear gloves for all PCR procedures.

1. Thaw the kit solutions. Mix thoroughly and centrifuge briefly
2. Prepare the reactions, as described below:

CONTENTS	N° OF SAMPLES	
qPCR reaction	1	10 (10 + 1)
Master Mix	16 µl	176 µl
Assay Mix – <i>eae</i> or Assay Mix – <i>vtx1</i> or Assay Mix – <i>vtx2</i>	2 µl	22 µl
Total Volume	18 µl	198 µl

Note: Prepare the PCR reaction for each sample, or in the alternative, prepare a Master Mix for the total number of reactions plus 10% to cover pipetting losses (e.g. for 10 samples, prepare a volume for 11). In this case, prepare the Mix in a 1,5mL sterile, nuclease-free tube. Include 2 PCR reactions for the Positive and Negative controls.

3. Mix the prepared Mix by inverting the tube and centrifuge briefly
4. Dispense 18 µL aliquots of prepared Mix into the plate wells or PCR tube
5. For the negative control, pipette 2 µL of Negative Control tube (Clear Cap); Pipette 2 µL of DNA sample per well; and for the positive control, pipette 2 µL of Positive Control tube (Red Cap). Each PCR tube / well should have a final PCR volume of 20 µL
6. Centrifuge briefly the plate wells or PCR tubes
7. Place the reactions into the Real Time PCR instrument.

B – Program set up

Prepare the Real-Time PCR instrument according to the following temperature/time program:

PHASE	STEP	TEMPERATURE	TIME	ACQUISITION
Holding Stage	Step 1	50°C	2 min.	No
	Step 2	95°C	5 min.	No
Amplification - 40 cycles	Step 1	95°C	30s	No
	Step 2	60°C	30s	Yes
	Step 3	72°C	30s	No

TARGET	CHANNELS
Detection of <i>E.coli eae</i> or <i>vtx1</i> or <i>vtx2</i>	FAM
Detection of Internal Control (IC)	ROX

11. DATA ANALYSIS

For analysis of PCR results, select fluorescence display options. Samples with positive Ct-values are considered positive.

Important: Please, also check amplification curves, not only Ct values. Samples should be inspected both in logarithmic and linear scale view and compared with the negative control. Adjust the Threshold, if necessary. Assessment of sample results should be performed after the positive and negative controls have been examined and determined to be valid. If the results of controls are not valid, the sample results cannot be interpreted. Interpretation of PCR data:

a) Controls

To validate the assay, the controls must have the following results:

	<i>E.coli eae</i> or <i>vtx1</i> or <i>vtx2</i> DETECTION FAM	IC DETECTION ROX
Negative Control	Negative	Positive
Positive Control	Positive	Positive

Note that if the controls do not match these results, the experiment must be repeated.

b) Samples

Interpretation of sample results is summarized in the following table:

<i>E.coli eae</i> or <i>vtx1</i> or <i>vtx2</i> DETECTION FAM	IC DETECTION ROX	INTERPRETATION
Positive	Positive/Negative**	DNA detected, sample Positive for <i>E.coli</i> (see table below)
Negative	Positive	No DNA detected, sample Negative for <i>E.coli</i>
Negative	Negative	Invalid Result*

*When both *E. coli* and IC detection are Negative, this means the presence of PCR inhibitors in the sample. Dilute the DNA sample (10-fold dilution) or perform another DNA extraction and repeat qPCR.

** High DNA concentration of the target in the sample can lead to a reduced or absent fluorescence signal of the IC.

Pathotype determination

<i>E.coli eae</i>	<i>E.coli vtx1</i>	<i>E.coli vtx2</i>	PATHOTYPE
Positive	Positive	Positive	EHEC
Positive	Positive	Negative	EHEC
Positive	Negative	Positive	EHEC
Positive	Negative	Negative	EPEC
Negative	Positive	Negative	VTEC
Negative	Negative	Positive	VTEC
Negative	Positive	Positive	VTEC